




User's Guide

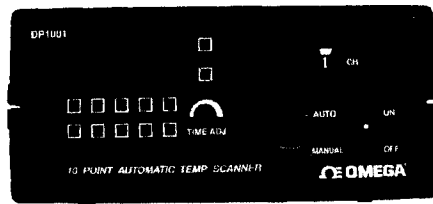

Shop online at

omega.com

www.omega.com
e-mail: info@omega.com



DP1001M & DP1001A 10-Channel Thermometer

OMEGAnet® Online Service www.omega.com	Internet e-mail info@omega.com
---	--

Servicing North America:

USA:
ISO 9001 Certified

One Omega Drive, Box 4047
Stamford CT 06907-0047
Tel: (203) 359-1660
e-mail: info@omega.com

FAX: (203) 359-7700

Canada:

976 Bergar
Laval (Quebec) H7L 5A1
Tel: (514) 856-6928
e-mail: info@omega.ca

FAX: (514) 856-6886

For immediate technical or application assistance:

USA and Canada: Sales Service: 1-800-826-6342 / 1-800-TC-OMEGA®
Customer Service: 1-800-622-2378 / 1-800-622-BEST®
Engineering Service: 1-800-872-9436 / 1-800-USA-WHEN®
TELEX: 996404 EASYLINK: 62968934 CABLE: OMEGA

Mexico:

En Español: (001) 203-359-7803
FAX: (001) 203-359-7807
TEL: (203) 359-1660

e-mail: espanol@omega.com
info@omega.com.mx

Servicing Europe:

Benelux: Postbus 8034, 1180 LA Amstelveen, The Netherlands
Tel: +31 (0)20 3472121 FAX: +31 (0)20 6434643
Toll Free in Benelux: 0800 0993344
e-mail: sales@omegaeng.nl

Czech Republic: Rudé armády 1868, 733 01 Karviná 8
Tel: +420 (0)69 6311899 FAX: +420 (0)69 6311114
Toll Free: 0800-1-66342 e-mail: czech@omega.com

France: 9, rue Denis Papin, 78190 Trappes
Tel: +33 (0)130 621 400 FAX: +33 (0)130 699 120
Toll Free in France: 0800-4-06342
e-mail: sales@omega.fr

Germany/Austria: Daimlerstrasse 26, D-75392 Deckenpfronn, Germany
Tel: +49 (0)7056 9398-0 FAX: +49 (0)7056 9398-29
Toll Free in Germany: 0800 639 7678
e-mail: info@omega.de , patient-connected applications.

United Kingdom: One Omega Drive, River Bend Technology Centre
ISO 9002 Certified Northbank, Irlam, Manchester
M44 5BD United Kingdom
Tel: +44 (0)161 777 6611 FAX: +44 (0)161 777 6622
Toll Free in United Kingdom: 0800-488-488
e-mail: sales@omega.co.uk

It is the policy of OMEGA to comply with all worldwide safety and EMC/EMI regulations that apply. OMEGA is constantly pursuing certification of its products to the European New Approach Directives. OMEGA will add the CE mark to every appropriate device upon certification.

The information contained in this document is believed to be correct, but OMEGA Engineering, Inc. accepts no liability for any errors it contains, and reserves the right to alter specifications without notice. WARNING: These products are not designed for use in, and should not be used for

TABLE OF CONTENTS

PAGE

1. INTRODUCTION	4
1.1 General Description	4
1.2 Accessories	4
2. GETTING STARTED	5
2.1 Unpacking	5
3. SAFETY CONSIDERATIONS	5
4. DISPLAY BACK AND FRONT PANEL	6
4.1 FRONT VIEW	6
4.2 BACK VIEW	7
5. OPERATING INSTRUCTIONS	8
6. CONSUMPTION	8
7. SPECIFICATIONS	8

TABLES AND PICTURES

Figure 4-1 Front view	6
Figure 4-2 Back view	7

1.0 INTRODUCTION

The DP1001M and the DP1001A are able to measure temperatures from 10 different locations and portray this information in a fashion very similar to watching television. Each location is assigned to a channel. To view the temperature of that location, you switch to that channel and its temperature will appear on the screen.

1.1 General Description

- DP1001A is an auto scan model, & DP1001M is a manual model.
- Both are bench type with a 10 channel selection.
- Different models in type K, Type J, and Type T are available for purchase use.
- Large & super bright LED display.
- °C/°F switchable with switch at rear & °C/°F indicator lamp in the front
- The channel switch is on the front panel, it is also easy to see the channel number displayed on the front panel.
- Sensors can be easily connected to input screw terminals at rear of case.
- Auto scanning channels with adjustable scan rate that goes from 2 to 16 seconds.

1.2 Accessories

DC 9V power adaptor

2.0 GETTING STARTED

2.1 Unpacking

Remove the packing list and verify that you have received all equipment. Upon receiving the shipment, inspect the container and equipment for any signs of damage.

Note: If there is any evidence of rough handling in transit, immediately report any damage to the shipping agent.

Note: The carrier will not honor any claims unless all shipping material is saved for their examination. After examining and removing contents, save packing materials and carton in the event reshipment is necessary.


3.0 SAFETY CONSIDERATIONS

This device is marked with the International Caution symbol. It is important to read this manual before installing or commissioning this device as it contains important information relating to Safety and EMC (Electromagnetic Compatibility).

- Do not exceed voltage rating on the label located on the top of the instrument housing.
- Always disconnect power before changing signal and power connections.
- Do not use this instrument on a work bench without it's case for safety reasons.
- Do not operate this instrument in flammable or explosive atmospheres.
- Do not expose this instrument to rain or moisture.

4.0 DISPLAY OF FRONT AND BACK PANEL

4.1 FRONT VIEW

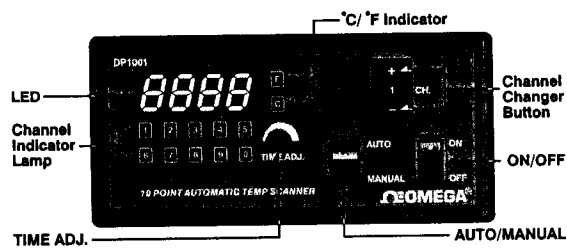

LED: This is the screen in which the temperature will appear.

°C/°F Indicator: These LED lamp whether you are seeing the temperature in Celsius or Fahrenheit.

Channel changer buttons: These buttons allow you to change the channel under MANUAL status. The positive button counts up and the negative button counts down.

Channel Indicator Lamp: These lights tell you which channel you have the thermometer set for.


ON/OFF : Switch ON or off.

AUTO/MANUAL : Switch for scanning with automation or manual.

TIME ADJ. : Adjust for channel scan rate under AUTO status.

4.0 DISPLAY OF FRONT AND BACK PANEL

4.2 BACK VIEW

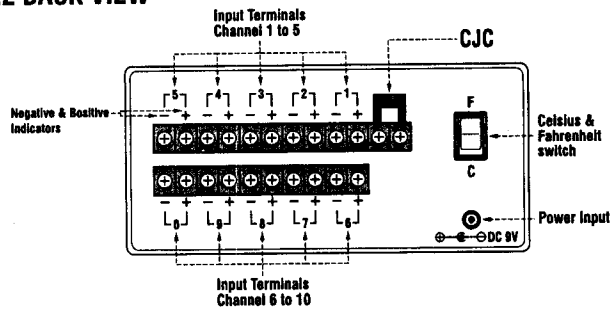

Negative & Positive Indicators: These are signs indicating where the positive and negative wires for each channel must go.

Input Terminals 1-10: These are the terminals where you will attach the wires. They are labeled according to the channels that the terminals represent.

Celsius & Fahrenheit switch: This switch allows you to change the units of measurement to either Celsius or Fahrenheit.

Power Input: This is the port where you must plug in the AC power adaptor provided with the package. The AC power adaptor is good only to receive power at 110 VAC and 60Hz.

CJC: Cold junction compensation

5.0 OPERATION INSTRUCTIONS

1. Connect the power source with AC adapter to the device and turn the device ON.
 2. You now must choose whether you want to read the temperature in Celsius or Fahrenheit.
 3. Wire the inputs according to wiring diagrams at the rear (10 input channel).
- NOTE:** Every TYPE compensation wire is different.
4. Switch mode to "AUTO" and adjust "TIME ADJ" for channel scan rate.
 5. Auto mode: (DP1001A only)
 - a. Adjust TIME ADJ to set desired scanning speed.
 - b. The channel changer buttons will not work on AUTO mode.
 - c. Scanner will automatically display temperature with LED channel indicators with desired scanning speed.
 6. Switch mode to "Manual" and thumb channel number which you need.

6.0 CONSUMPTION

Wattage: 26mA X 110V = 2.9W

7.0 SPECIFICATIONS

	Type J	Type K	Type T
Range:	-50 to 700°C (50 to 1400°F)	0 to 1200°C (0 to 1999°F)	-50 to 350°C (-58 to 662°F)
Resolution:	1°C/F	1°C/F	1°C/F
Accuracy:	0.25% FS	0.25% FS	0.25% FS
Power:	DC 9V with AC adaptor		
Dimensions:	180 x 76 x 145 mm (7.1 x 3.0 x 5.7")		
Weight:	964g (2.1 oz.)		

WARRANTY/DISCLAIMER

OMEGA ENGINEERING, INC. warrants this unit to be free of defects in materials and workmanship for a period of 13 months from date of purchase. OMEGA's Warranty adds an additional one (1) month grace period to the normal one (1) year product warranty to cover handling and shipping time. This ensures that OMEGA's customers receive maximum coverage on each product.

If the unit malfunctions, it must be returned to the factory for evaluation. OMEGA's Customer Service Department will issue an Authorized Return (AR) number immediately upon phone or written request. Upon examination by OMEGA, if the unit is found to be defective, it will be repaired or replaced at no charge. OMEGA's WARRANTY does not apply to defects resulting from any action of the purchaser, including but not limited to mishandling, improper interfacing, operation outside of design limits, improper repair, or unauthorized modification. This WARRANTY is VOID if the unit shows evidence of having been tampered with or shows evidence of having been damaged as a result of excessive corrosion; or current, heat, moisture or vibration; improper specification; misapplication; misuse or other operating conditions outside of OMEGA's control. Components which wear are not warranted, including but not limited to contact points, fuses, and triacs, conduct(s) in such a manner.

OMEGA is pleased to offer suggestions on the use of its various products. However, OMEGA neither assumes responsibility for any omissions or errors nor assumes liability for any damages that result from the use of its products in accordance with information provided by OMEGA, either verbal or written. OMEGA warrants only that the parts manufactured by it will be as specified and free of defects. OMEGA MAKES NO OTHER WARRANTIES OR REPRESENTATIONS OF ANY KIND WHATSOEVER, EXPRESS OR IMPLIED, EXCEPT THAT OF TITLE, AND ALL IMPLIED WARRANTIES INCLUDING ANY WARRANTY OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE ARE HEREBY DISCLAIMED. LIMITATION OF LIABILITY: The remedies of purchaser set forth herein are exclusive, and the total liability of OMEGA with respect to this order, whether based on contract, warranty, negligence, indemnification, strict liability or otherwise, shall not exceed the purchase price of the component upon which liability is based. In no event shall OMEGA be liable for consequential, incidental or special damages.

CONDITIONS: Equipment sold by OMEGA is not intended to be used, nor shall it be used (1) as a "Basic Component" under 10 CFR 21 (NRC), used in or with any nuclear installation or activity; or (2) in medical applications or used on humans. Should any Product(s) be used in or with any nuclear installation or activity, medical application, used on humans, or misused in any way, OMEGA assumes no responsibility as set forth in our basic WARRANTY/DISCLAIMER language, and, additionally, purchaser will indemnify OMEGA and hold OMEGA harmless from any liability or damage whatsoever arising out of the use of the Product(s) in such a manner.

RETURN REQUESTS/INQUIRIES

Direct all warranty and repair requests/inquiries to the OMEGA Customer Service Department. BEFORE RETURNING ANY PRODUCT(S) TO OMEGA, PURCHASER MUST OBTAIN AN AUTHORIZED RETURN (AR) NUMBER FROM OMEGA'S CUSTOMER SERVICE DEPARTMENT (IN ORDER TO AVOID PROCESSING DELAYS). The assigned AR number should then be marked on the outside of the return package and on any correspondence.

The purchaser is responsible for shipping charges, freight, insurance and proper packaging to prevent breakage in transit.

FOR **WARRANTY** RETURNS, please have the following information available BEFORE contacting OMEGA:

1. Purchase Order number under which the product was PURCHASED,
2. Model and serial number of the product under warranty, and
3. Repair instructions and/or specific problems relative to the product. ENGINEERING, INC.

FOR **NON-WARRANTY** REPAIRS, consult OMEGA for current repair charges. Have the following information available BEFORE contacting OMEGA:

1. Purchase Order number to cover the COST of the repair,
2. Model and serial number of the product, and
3. Repair instructions and/or specific problems relative to the product.

OMEGA's policy is to make running changes, not model changes, whenever an improvement is possible. This affords our customers the latest in technology and engineering.

OMEGA is a registered trademark of OMEGA ENGINEERING, INC.

© Copyright 2001 OMEGA ENGINEERING, INC. All rights reserved. This document may not be copied, photocopied, reproduced, translated, or reduced to any electronic medium or machine-readable form, in whole or in part, without the prior written consent of OMEGA

**Where Do I Find Everything I Need for
Process Measurement and Control?
OMEGA...Of Course!**

Shop online at www.omega.com

TEMPERATURE

- Thermocouple, RTD & Thermistor Probes, Connectors, Panels & Assemblies
- Wire: Thermocouple, RTD & Thermistor
- Calibrators & Ice Point References
- Recorders, Controllers & Process Monitors
- Infrared Pyrometers

PRESSURE, STRAIN AND FORCE

- Transducers & Strain Gages
- Load Cells & Pressure Gages
- Displacement Transducers
- Instrumentation & Accessories

FLOW/LEVEL

- Rotameters, Gas Mass Flowmeters & Flow Computers
- Air Velocity Indicators
- Turbine/Paddlewheel Systems
- Totalizers & Batch Controllers

pH/CONDUCTIVITY

- pH Electrodes, Testers & Accessories
- Benchtop/Laboratory Meters
- Controllers, Calibrators, Simulators & Pumps
- Industrial pH & Conductivity Equipment

DATA ACQUISITION

- Data Acquisition & Engineering Software
- Communications-Based Acquisition Systems
- Plug-in Cards for Apple, IBM & Compatibles
- Datalogging Systems
- Recorders, Printers & Plotters

HEATERS

- Heating Cable
- Cartridge & Strip Heaters
- Immersion & Band Heaters
- Flexible Heaters
- Laboratory Heaters

**ENVIRONMENTAL
MONITORING AND CONTROL**

- Metering & Control Instrumentation
- Refractometers
- Pumps & Tubing
- Air, Soil & Water Monitors
- Industrial Water & Wastewater Treatment
- pH, Conductivity & Dissolved Oxygen Instruments

M3754/1101