



5

**To Set the Decimal Point**


1. If it's not already shown, press MENU until the unit displays:




2. Press ► /DEV. The unit displays:



3. Press ▲ /MAX to move the decimal point to the desired location. The choices are FFFF. and FFF.F.




4. Press MENU to select the decimal point position shown. The unit displays:

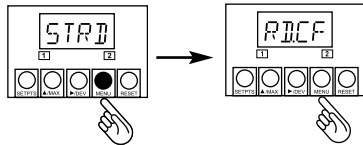


**To Set the Temperature Unit (Fahrenheit or Celsius):**


1. If it's not already shown, press MENU until the unit displays:




2. Press ► /DEV. The unit displays:



3. Press ▲ /MAX to display the setting you want. Choices are F and C.




4. Press MENU to select the temperature until shown. The unit displays:

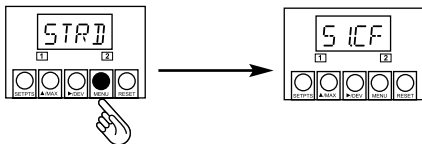

6

**Begin Operation**

Exit the Configuration MENU and reinitialize the meter.




- Press RESET twice, or
- Press MENU until RST flashes on the display.

When the temperature appears, the meter is up and running.

**Changing Setpoint Values**


1. While in RUN mode, press SETPTS. The controller displays the current value for setpoint 1:

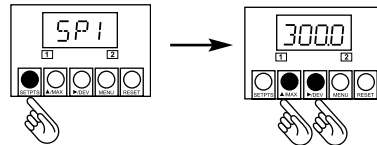

You can change setpoint 1 or press SETPTS again to show the current value for setpoint 2.


2. To change the setpoint 1 value:

- Press ► /DEV until the digit(s) you want to change flashes on the display.
- Press ▲ /MAX to change the value.
- Press SETPTS to store the value shown. The current value for setpoint 2 is shown:



3. Change setpoint 2 using the procedure above, or just press SETPTS to return to RUN mode.

**WARNING:** These products are not designed for use in, and should not be used for, patient connected applications.



It is the policy of OMEGA to comply with all worldwide safety and EMC/EMI regulations that apply. OMEGA is constantly pursuing certification of its products to the European New Approach Directives. OMEGA will add the mark to every appropriate device upon certification.

The information contained in this document is believed to be correct but OMEGA Engineering, Inc. accepts no liability for any errors it contains, and reserves the right to alter specifications without notice.

**TRADEMARK NOTICE:** *omega.com*<sup>™</sup>, and **OMEGA**<sup>®</sup>, are trademarks of OMEGA Engineering, Inc.

**MADE IN USA WARRANTY/DISCLAIMER**

OMEGA ENGINEERING, INC. warrants this unit to be free of defects in materials and workmanship for a period of **one (1) year** from the date of purchase. In addition to OMEGA's standard warranty period, OMEGA Engineering will extend the warranty period for **four (4) additional years** if the warranty card enclosed with each instrument is returned to OMEGA.

If the unit should malfunction, it must be returned to the factory for evaluation. OMEGA's Customer Service Department will issue an Authorized Return (AR) number immediately upon phone or written request. Upon examination by OMEGA, if the unit is found to be defective it will be repaired or replaced at no charge. Omega's WARRANTY does not apply to defects resulting from any action of the purchaser, including but not limited to mishandling, improper interfacing, operation outside of design limits, improper repair, or unauthorized modification. This WARRANTY is VOID if the unit shows evidence of having been tampered with or shows evidence of being damaged as a result of excessive corrosion; or current, heat, moisture or vibration; improper specification; misapplication; misuse or other operating conditions outside of OMEGA's control. Components which wear are not warranted, including but not limited to contact points, fuses, and triacs.

**OMEGA is pleased to offer suggestions on the use of its various products. However, OMEGA neither assumes responsibility for any omissions or errors nor assumes liability for any damages that result from the use of its products in accordance with information provided by OMEGA, either verbal or written. OMEGA warrants only that the parts manufactured by it will be as specified and free of defects. OMEGA MAKES NO OTHER WARRANTIES OR REPRESENTATIONS OF ANY KIND WHATSOEVER, EXPRESSED OR IMPLIED, EXCEPT THAT OF TITLE, AND ALL IMPLIED WARRANTIES INCLUDING ANY WARRANTY OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE ARE HEREBY DISCLAIMED. LIMITATION OF LIABILITY: The remedies of purchaser set forth herein are exclusive and the total liability of OMEGA with respect to this order, whether based on contract, warranty, negligence, indemnification, strict liability or otherwise, shall not exceed the purchase price of the component upon which liability is based. In no event shall OMEGA be liable for consequential, incidental or special damages.**

CONDITIONS: Equipment sold by OMEGA is not intended to be used, nor shall it be used: (1) as a "Basic Component" under 10 CFR 21 (NRC), used in or with any nuclear installation or activity; or (2) in medical applications or used on humans. Should any Product(s) be used in or with any nuclear installation or activity, medical application, used on humans, or misused in any way, OMEGA assumes no responsibility as set forth in our basic WARRANTY / DISCLAIMER language, and additionally, purchaser will indemnify OMEGA and hold OMEGA harmless from any liability or damage whatsoever arising out of the use of the Product(s) in such a manner.

**RETURN REQUESTS / INQUIRIES**

Direct all warranty and repair requests/inquiries to the OMEGA Customer Service Department. **BEFORE RETURNING ANY PRODUCT(S) TO OMEGA, PURCHASER MUST OBTAIN AN AUTHORIZED RETURN (AR) NUMBER FROM OMEGA'S CUSTOMER SERVICE DEPARTMENT (IN ORDER TO AVOID PROCESSING DELAYS).** The assigned AR number should then be marked on the outside of the return package and on any correspondence.

The purchaser is responsible for shipping charges, freight, insurance and proper packaging to prevent breakage in transit.

FOR **WARRANTY** RETURNS, please have the following information available **BEFORE** contacting OMEGA:

1. P.O. number under which the product was PURCHASED,
2. Model and serial number of the product under warranty, and
3. Repair instructions and/or specific problems relative to the product.

FOR **NON-WARRANTY** REPAIRS, consult OMEGA for current repair charges. Have the following information available **BEFORE** contacting OMEGA:

1. P.O. number to cover the COST of the repair,
2. Model and serial number of product, and
3. Repair instructions and/or specific problems relative to the product.

OMEGA's policy is to make running changes, not model changes, whenever an improvement is possible. This affords our customers the latest in technology and engineering.

OMEGA is a registered trademark of OMEGA ENGINEERING, INC. © Copyright 2006 OMEGA ENGINEERING, INC. All rights reserved. This document may not be copied, photocopied, reproduced, translated, or reduced to any electronic medium or machine-readable form, in whole or in part, without prior written consent of OMEGA ENGINEERING, INC.

**PATENT NOTICE:** The "Meter Case Bezel Design" is a trademark of NEWPORT Electronics, Inc., registered in the U.S. USED UNDER LICENSE. This product is covered by one or more of the following patents: U.S. Pat. No. Des. 336,895; 5,274,577 / CANADA 2052599; 2052600 / ITALY 1249456; 1250938 / FRANCE BREVET No. 91 12756 / SPAIN 2039150; 2048066 / UK PATENT No. GB2 249 837; GB2 248 954 / GERMANY DE 41 34398 C2. OTHER INTERNATIONAL PATENTS PENDING.

**QUICK START**

**RoHS 2 Compliant**



**CN1001-TC Temperature Controller with Time Proportional Control**



<b>OMEGAnet<sup>®</sup> On-Line Service</b> <a href="http://www.omega.com">www.omega.com</a>	<b>Internet e-mail</b> <a href="mailto:info@omega.com">info@omega.com</a>
---	--

**Servicing North America:**

**USA:** One Omega Drive, P.O. Box 4047  
Stamford CT 06907-0047  
ISO 9001 Certified TEL: (203) 359-1660 FAX: (203) 359-7700  
e-mail: [info@omega.com](mailto:info@omega.com)

**Canada:** 976 Bergar  
Laval (Quebec) H7L 5A1  
TEL: (514) 856-6928 FAX: (514) 856-6886  
e-mail: [info@omega.ca](mailto:info@omega.ca)

**For immediate technical or application assistance:**

**USA and Canada:** Sales Service: 1-800-826-6342 / 1-800-TC-OMEGA<sup>®</sup>  
Customer Service: 1-800-622-2378 / 1-800-622-BEST<sup>®</sup>  
Engineering Service: 1-800-872-9436 / 1-800-USA-WHEN<sup>®</sup>

**Mexico and Latin American:** TEL: (001)800-TC-OMEGA<sup>®</sup> FAX: (001) 203-359-7807  
En Español: (001) 203-359-7803  
e-mail: [espanol@omega.com](mailto:espanol@omega.com)

**Servicing Europe:**

**Czech Republic:** Frystatska 184, 733 01 Karviná  
TEL: +420 59 6311899 FAX: +420 59 6311114  
e-mail: [info@omegashop.cz](mailto:info@omegashop.cz)

**Germany/Austria:** Daimlerstrasse 26, D-75392 Deckenpfronn, Germany  
TEL: +49 7056 9398-0 FAX: +49 7056 9398-29  
Toll Free in Germany: 0800 639 7678  
e-mail: [info@omega.de](mailto:info@omega.de)

**United Kingdom:** One Omega Drive  
ISO 9002 Certified River Bend Technology Centre  
Northbank, Irlam Manchester M44 5BD United Kingdom  
TEL: +44 161 777 6611 FAX: +44 161 777 6622  
Toll Free in England: 0800 488 488  
e-mail: [sales@omega.co.uk](mailto:sales@omega.co.uk)

## Using This Quick Start Manual

Use this Quick Start Manual to set up your Controller and begin operation. Information is provided on how to:

- Connect ac power
- Connect the thermocouple
- Set basic options for operation

For complete information on all setup options, please refer to the Operator's Manual.


## Before You Begin

In addition to the controller and the related parts, you will need the following items to set up your unit:

- ac power, as listed on the units ID/Product Label
- Thermocouple
- 1/8-inch flat-blade screwdriver.

## Mount the Unit


1. Cut a panel opening using the dimensions shown to the right.
2. Position the unit in the opening, making sure the front bezel gasket is flush to the panel.
3. Slide on mounting bracket to secure.

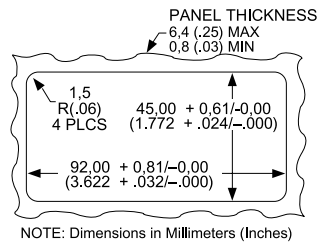

**Warning:** Do not connect ac power to your meter until you have completed all input and output connections. Failure to do so may result in injury!

## Connect AC Power


1. Remove the panel at the back of the unit.
2. Locate the TB1 connector.
3. Insert the correct wire in each terminal as shown in the following figure and tighten the lockdown screws.
4. Tug gently on the wires to verify the connections.

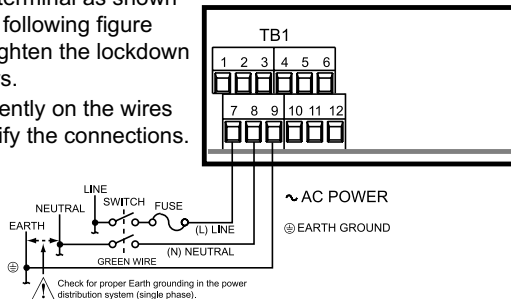


## Main ac Power Connections

## Connect the Thermocouple

1. Locate the Thermocouple connector on the rear of the unit. Refer figure below for location.

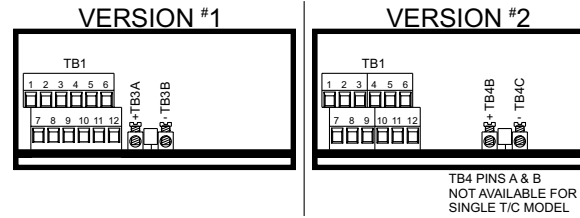

2. Attach the thermocouple wires.
  - Connect positive (+) lead of thermocouple.
  - Connect negative (-) red lead of thermocouple.
3. Tighten the lockdown screws. The following figure shows the correct wiring.
4. Tug gently on the wires to verify the connections.
5. Replace the panel at the back of the unit.

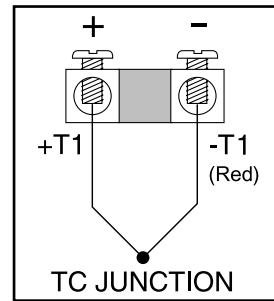

## Thermocouple Input Connection

## Turn On the Unit

1. Apply ac power to the unit.
 

As the unit initializes, flashing RST and then T/C on the front panel. Then the temperature should appear.
2. Verify that a temperature is displayed. If not:
  - Remove ac power
  - Verify the TB1 power connections
  - Check your power source
  - Apply ac power again.


## Configure the Unit

To configure the unit, you use the buttons on the front panel.


To:	Take This Action:
Display the Configuration Menu	Press the MENU button. The first on the menu, INPT, displays.
Select a submenu function	<ol style="list-style-type: none"> <li>1. Press MENU until the function you want is shown.</li> <li>2. Press ► /DEV.</li> </ol> <p>The information you can change begins to flash.</p>
Select a value for that submenu function	<ol style="list-style-type: none"> <li>1. Press ▲ /MAX to display the option you want.</li> <li>2. Press MENU to select it.</li> </ol> <p>The message STRD quickly flashes, indicating that the selection has been stored in memory. Then the next menu function displays.</p>
Go back to the previous menu function	Press RESET once.
Exit the Configuration	<p>Press RESET twice. The unit reinitializes (displays RST, then T/C). When the temperature displays, the unit is back in run mode.</p> <p>(Optionally, you can press MENU to move through all the menu functions until the unit reinitializes.)</p>

## To Set the Thermocouple Type:


1. Press MENU until the unit displays:



2. Press ► /DEV. The unit displays:



3. Press ▲ /MAX until the thermocouple for your installation is shown.



Choices are J.TC, K.TC, T.TC, DJ.TC

4. Press MENU to select the thermocouple shown. The unit displays:

