



WARRANTY/DISCLAIMER

OMEGA ENGINEERING, INC. warrants this unit to be free of defects in materials and workmanship for a period of **25 months** from date of purchase of the **base unit** and **13 months** from date of purchase on **Laser Sight Module**. OMEGA's WARRANTY adds an additional one (1) month grace period to the normal **one (1) year product warranty** to cover handling and shipping time. This ensures that OMEGA's customers receive maximum coverage on each product.

If the unit malfunctions, it must be returned to the factory for evaluation. OMEGA's Customer Service Department will issue an Authorized Return (AR) number immediately upon phone or written request. Upon examination by OMEGA, if the unit is found to be defective, it will be repaired or replaced at no charge. OMEGA's WARRANTY does not apply to defects resulting from any action of the purchaser, including but not limited to mishandling, improper interfacing, operation outside of design limits, improper repair, or unauthorized modification. This WARRANTY is VOID if the unit shows evidence of having been tampered with or shows evidence of having been damaged as a result of excessive corrosion; or current, heat, moisture or vibration; improper specification; misapplication; misuse or other operating conditions outside of OMEGA's control. Components in which wear are not warranted, include but are not limited to contact points, fuses, and triacs.

OMEGA is pleased to offer suggestions on the use of its various products. However, OMEGA neither assumes responsibility for any omissions or errors nor assumes liability for any damages that result from the use of its products in accordance with information provided by OMEGA, either verbal or written. OMEGA warrants only that the parts manufactured by the company will be as specified and free of defects. OMEGA MAKES NO OTHER WARRANTIES OR REPRESENTATIONS OF ANY KIND WHATSOEVER, EXPRESSED OR IMPLIED, EXCEPT THAT OF TITLE, AND ALL IMPLIED WARRANTIES INCLUDING ANY WARRANTY OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE ARE HEREBY DISCLAIMED. LIMITATION OF LIABILITY: The remedies of purchaser set forth herein are exclusive, and the total liability of OMEGA with respect to this order, whether based on contract, warranty, negligence, indemnification, strict liability or otherwise, shall not exceed the purchase price of the component upon which liability is based. In no event shall OMEGA be liable for consequential, incidental or special damages.

CONDITIONS: Equipment sold by OMEGA is not intended to be used, nor shall it be used: (1) as a "Basic Component" under 10 CFR 21 (NRC), used in or with any nuclear installation or activity; or (2) in medical applications or used on humans. Should any Product(s) be used in or with any nuclear installation or activity, medical application, used on humans, or misused in any way, OMEGA assumes no responsibility as set forth in our basic WARRANTY/DISCLAIMER language, and, additionally, purchaser will indemnify OMEGA and hold OMEGA harmless from any liability or damage whatsoever arising out of the use of the Product(s) in such a manner.

RETURN REQUESTS/INQUIRIES

Direct all warranty and repair requests/inquiries to the OMEGA Customer Service Department. BEFORE RETURNING ANY PRODUCT(S) TO OMEGA, PURCHASER MUST OBTAIN AN AUTHORIZED RETURN (AR) NUMBER FROM OMEGA'S CUSTOMER SERVICE DEPARTMENT (IN ORDER TO AVOID PROCESSING DELAYS). The assigned AR number should then be marked on the outside of the return package and on any correspondence.

FOR **WARRANTY** RETURNS, please have the following information available BEFORE contacting OMEGA:

1. Purchase Order number under which the product was PURCHASED,
2. Model and serial number of the product under warranty, and
3. Repair instructions and/or specific problems relative to the product.

FOR **NON-WARRANTY** REPAIRS, consult OMEGA for repair charges. Have the following information available BEFORE contacting OMEGA:

1. Purchase Order number to cover the COST of the repair or calibration,
2. Model and serial number of the product, and
3. Repair instructions and/or specific problems relative to the product.

OMEGA's policy is to make running changes, not model changes, whenever an improvement is possible. This affords our customers the latest in technology and engineering.


OMEGA is a registered trademark of OMEGA ENGINEERING, INC.

© Copyright 2005 OMEGA ENGINEERING, INC. All rights reserved. This document may not be copied, photocopied, reproduced, translated, or reduced to any electronic medium or machine-readable form, in whole or in part, without the prior written consent of OMEGA ENGINEERING, INC.

5

Functional Flow Chart when the Trigger is Pulled (Real Time Mode)

Real Time Modes	Press to...	Press to...	Display shows:
DISPLAY MODE: E	Go to	Lock or unlock Trigger LOCK	Emissivity Current temperature
DISPLAY MODE: E/F	Go to	Set laser to Flashing or On	Distance (feet or meter) Current temperature
DISPLAY MODE: LSR	Go to	Reset Maximum, Minimum, Diff. Average temps	Laser status Current temperature
DISPLAY MODE: MAX	Go to	Enable/Disable HAL	Maximum temperature Current temperature
DISPLAY MODE: MIN	Go to	Enable/Disable LAL	Minimum temperature Current temperature
DISPLAY MODE: DIF	Go to	Enable/Disable AIC	Differential temp Current temperature
DISPLAY MODE: AVG	Go to	Enable/Disable PRN	Average temperature Current temperature
DISPLAY MODE: HAL	Go to	Store temp data	High alarm set point Current temperature
DISPLAY MODE: LAL	Go to	Turn on/off Logging	Thermocouple temp Current temperature
DISPLAY MODE: AMB	Go to		Low alarm set point Current temperature
DISPLAY MODE: PRN	Go to		Ambient target temp Current temperature
DISPLAY MODE: MEM	Go to		Data Trans. Interval Current temperature
DISPLAY MODE: LOG	Go to		Memory location Current temperature
			Logging Current temperature




It is the policy of OMEGA to comply with all worldwide safety and EMC/EMI regulations that apply. OMEGA is constantly pursuing certification of its products to the European New Approach Directives. OMEGA will add the CE mark to every appropriate device upon certification.

The information contained in this document is believed to be correct but OMEGA Engineering, Inc. accepts no liability for any errors it contains, and reserves the right to alterspecifications without notice.

WARNING: These products are not designed for use in, and should not be used for, patient connected applications.


PATENT NOTICE This product may be protected by one or more of the following patents: U.S. PAT. D357,194; B1 5,368,392; 5,524,984; 5,727,880; 5,465,838; 5,823,678; 5,823,679; 6,123,453; 6,267,500 B1; 6,341,891 B1; 6,377,400 B1; 6,540,398 B2; 6,614,830 B1; 6,633,434 B2; 6,659,639; / Canada 2,114,806; 2,116,055; 75811 © OMEGA ENGINEERING, INC./ Czech Republic 25372/ France 2 756 920; 2 767 921; 2,773,213; 0378411 to 0378446; 2 773 213 B1 / Germany M 94 06 478.4; G 94 22 197.9; G 94 22 203.7/ Italy RM940000913/ Japan 988,378/Holland 1007752; 25009-00/ Spain mod. ut. 0133292/ Slovak Republic 24565/ U.K. Registered 2041153; 9726133.3/ EPO 0 644,408 B2; EP 1 085 307 A1. Other U.S. and Foreign Patents Pending. Other U.S. and International Patents Pending.

6

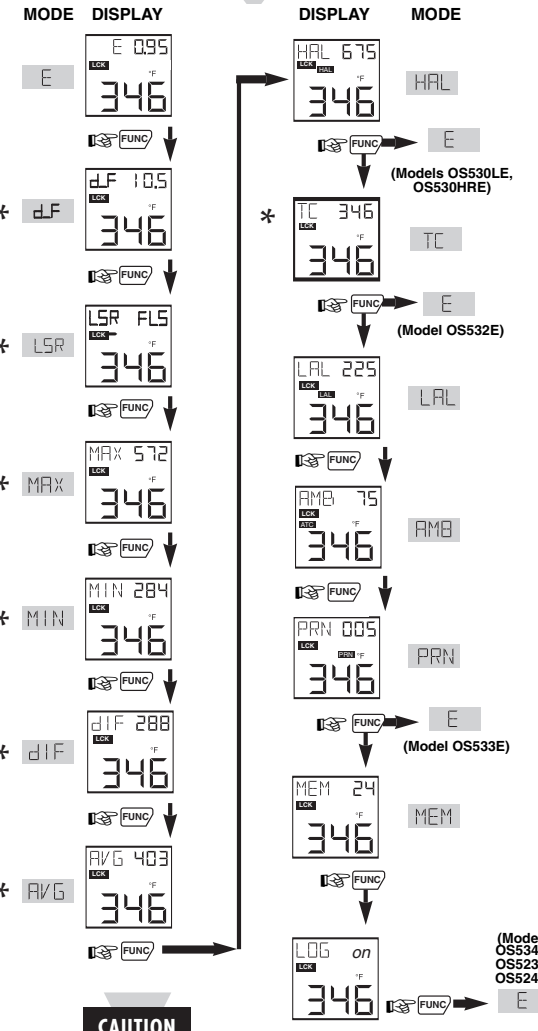

NOTE: The unit of measure (°F or °C) flashes during Real Time Mode.

- There should be a clean, open line of sight from the distance device to the target, otherwise an erroneous reading will result.
- For accurate distance measurement readings, the surface must be hard, flat, and reflective to ultrasonic pulse.
- Distance measurement can not be taken through glass, or off of soft and padded surfaces, or through smoke or fog.
- The distance measurement unit must be held perpendicular to the target surface.
- The distance measurement unit is designed for indoor use only.
- Accuracy of the distance measurement unit will vary depending on environmental conditions.
- Do not aim the distance measurement unit.



Warning and Certification Label

QUICK START

- OS530LE
- OS532E
- OS533E
- OS534E
- OS530HRE
- OS53x-CF
- OS523E
- OS524E



OMEGASCOPE® Handheld Infrared Thermometer



OMEGAnet® Online Service omega.com Internet e-mail info@omega.com

Servicing North America:
 U.S.A.: One Omega Drive, Box 4047
 ISO 9001 Certified Stamford, CT 06907-0047
 Tel: (203) 359-1660 FAX: (203) 359-7700
 e-mail: info@omega.com

Canada: 976 Bergar
 Laval (Quebec) H7L 5A1, Canada
 Tel: (514) 856-6928 FAX: (514) 856-6886
 e-mail: info@omega.ca

For immediate technical or application assistance:
 U.S.A. and Canada: Sales Service: 1-800-826-6342/1-800-TC-OMEGA®
 Customer Service: 1-800-622-2378/ 1-800-622-BEST®
 Engineering Service: 1-800-872-9436/1-800-USA-WHEN®

Mexico: En Español: (001) 203-359-7803
 e-mail: espanol@omega.com
 FAX: (001) 203-359-7807 info@omega.com.mx

Servicing Europe:
 Benelux: Postbus 8034, 1180 LA Amstelveen, The Netherlands
 Tel: +31 (0)20 3472121 FAX: +31 (0)20 6434643
 Toll Free in Benelux: 0800 0993344
 e-mail: sales@omegaeng.nl

Czech Republic: Frystatska 184, 733 01 Karvina, Czech Republic
 Tel: +420 (0)59 6311899 FAX: +420 (0)59 6311114
 Toll Free: 0800-1-66342 e-mail: info@omegashop.cz

France: 11, rue Jacques Cartier, 78280 Guyancourt, France
 Tel: +33 (0)1 61 37 2900 FAX: +33 (0)1 30 57 5427
 Toll Free in France: 0800 466 342
 e-mail: sales@omega.fr

Germany/Austria: Daimlerstrasse 26, D-75392 Deckenfronn, Germany
 Tel: +49 (0)7056 9398-0 FAX: +49 (0)7056 9398-29
 Toll Free in Germany: 0800 639 7678
 e-mail: info@omega.de

United Kingdom: One Omega Drive, River Bend Technology Centre
 ISO 9002 Certified Northbank, Irlam, Manchester
 M44 5BD United Kingdom
 Tel: +44 (0)161 777 6611 FAX: +44 (0)161 777 6622
 Toll Free in United Kingdom: 0800-488-488
 e-mail: sales@omega.co.uk

START HERE

Using this Quick Start Manual

Use this Quick Start Manual with your OS530E/ OS520E series Handheld Infrared Thermometer to set up and perform basic operations. These tasks are:

- Installing the Batteries
- Operating the Laser Sight
- Taking Temperature Readings
- Measuring Distance

For detailed information, refer to the User's Guide (M4088).

Getting Started

Parts of the Thermometer

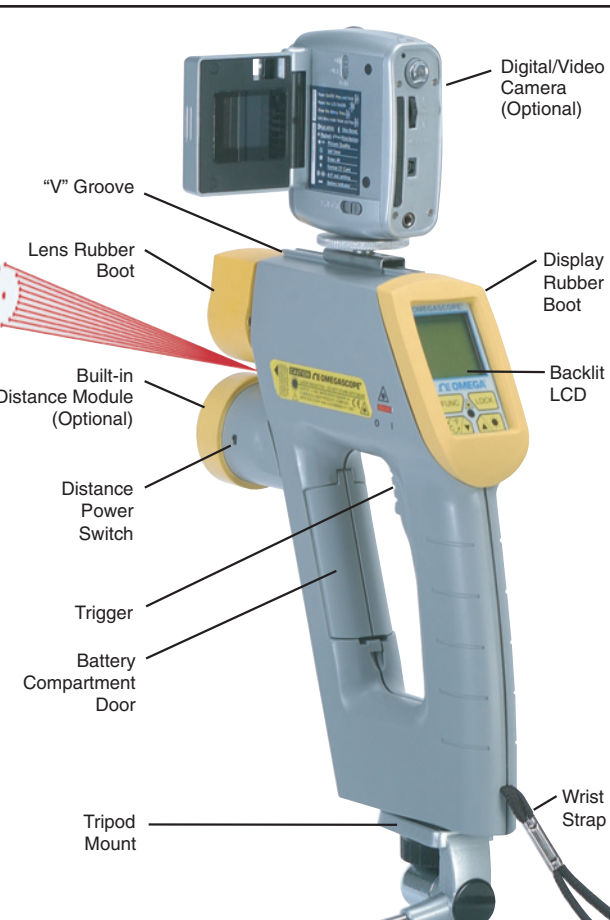


Figure 1. OS530E/OS520E Series Handheld Infrared Thermometer Front View



Figure 2. OS530E/OS520E Series Handheld Infrared Thermometer Various Views

2

3

4

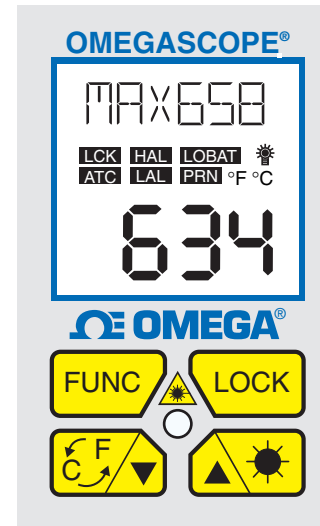


Figure 3. Display and Keypad View

Installing the Batteries

Invert the unit and install 4 fresh AA size batteries as shown in Figure 4.

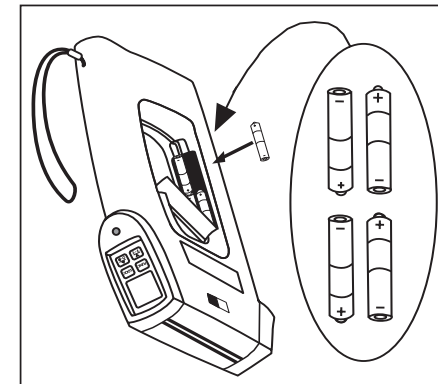


Figure 4. Installing the Batteries

Operating the Laser Sight Function

WARNING: DO NOT AIM THE LASER BEAM AT ANYONE'S EYES.

CAUTION: Use of controls or adjustments or performance of procedures other than those specified here may result in hazardous radiation exposure. Refer to the Operator's Manual for complete warnings and cautions.

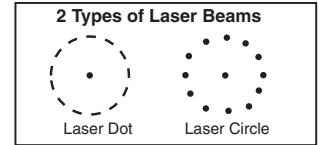


Figure 5. Two Laser Configurations
The thermometer is ready for operation.

Taking Temperature Readings

1. Aim at the target. If you are not using the Laser Sighting, use the "V" groove on top of the thermometer to align the target to the thermometer's field of view.

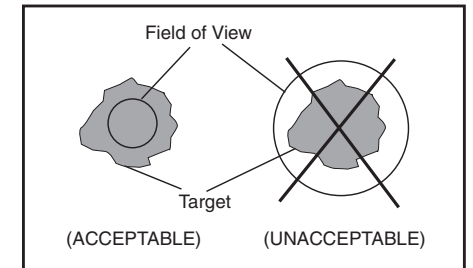


Figure 6. Field of View Positions

2. Pull and hold the trigger. To use the laser sighting, set the laser power switch to the ON position. The Power Indicator LED and the laser beam will turn on. The laser beam will stay on as long as the trigger is pulled. The target temperature and emissivity (E) will be displayed on the LCD. You can press the and key to increment or decrement the target emissivity. The laser beam is switchable between dot and circle using the switch on the right side.

Measuring Distance

Distance measurement is offered either as field mountable or built-in. The field mountable version (HH-DM) is a stand alone device. Press the key to measure distance. The built-in version (-DM) is an integral part of the thermometer. Go to the d_F or d_M display menu. Set the power switch on the distance module to the ON position. Pull the trigger for about 2 seconds. The upper display will show the distance in feet or meters. Releasing the trigger will turn off distance measurement.